R2P® Destination Slender®
Guiding Sheath

INTERVENE WITH **INCREASED SUPPORT**

Enhance your radial device algorithm with a thin-wall guiding sheath designed to provide support to your interventional procedures

- TERUMO Slender Technology™ reduces the outer diameter while maintaining an equivalent larger inner diameter
- Full hydrophilic coating designed to minimize vessel spasm at access site[1]
- Device lengths designed to support coronary, neuro, visceral, and peripheral procedures[a]

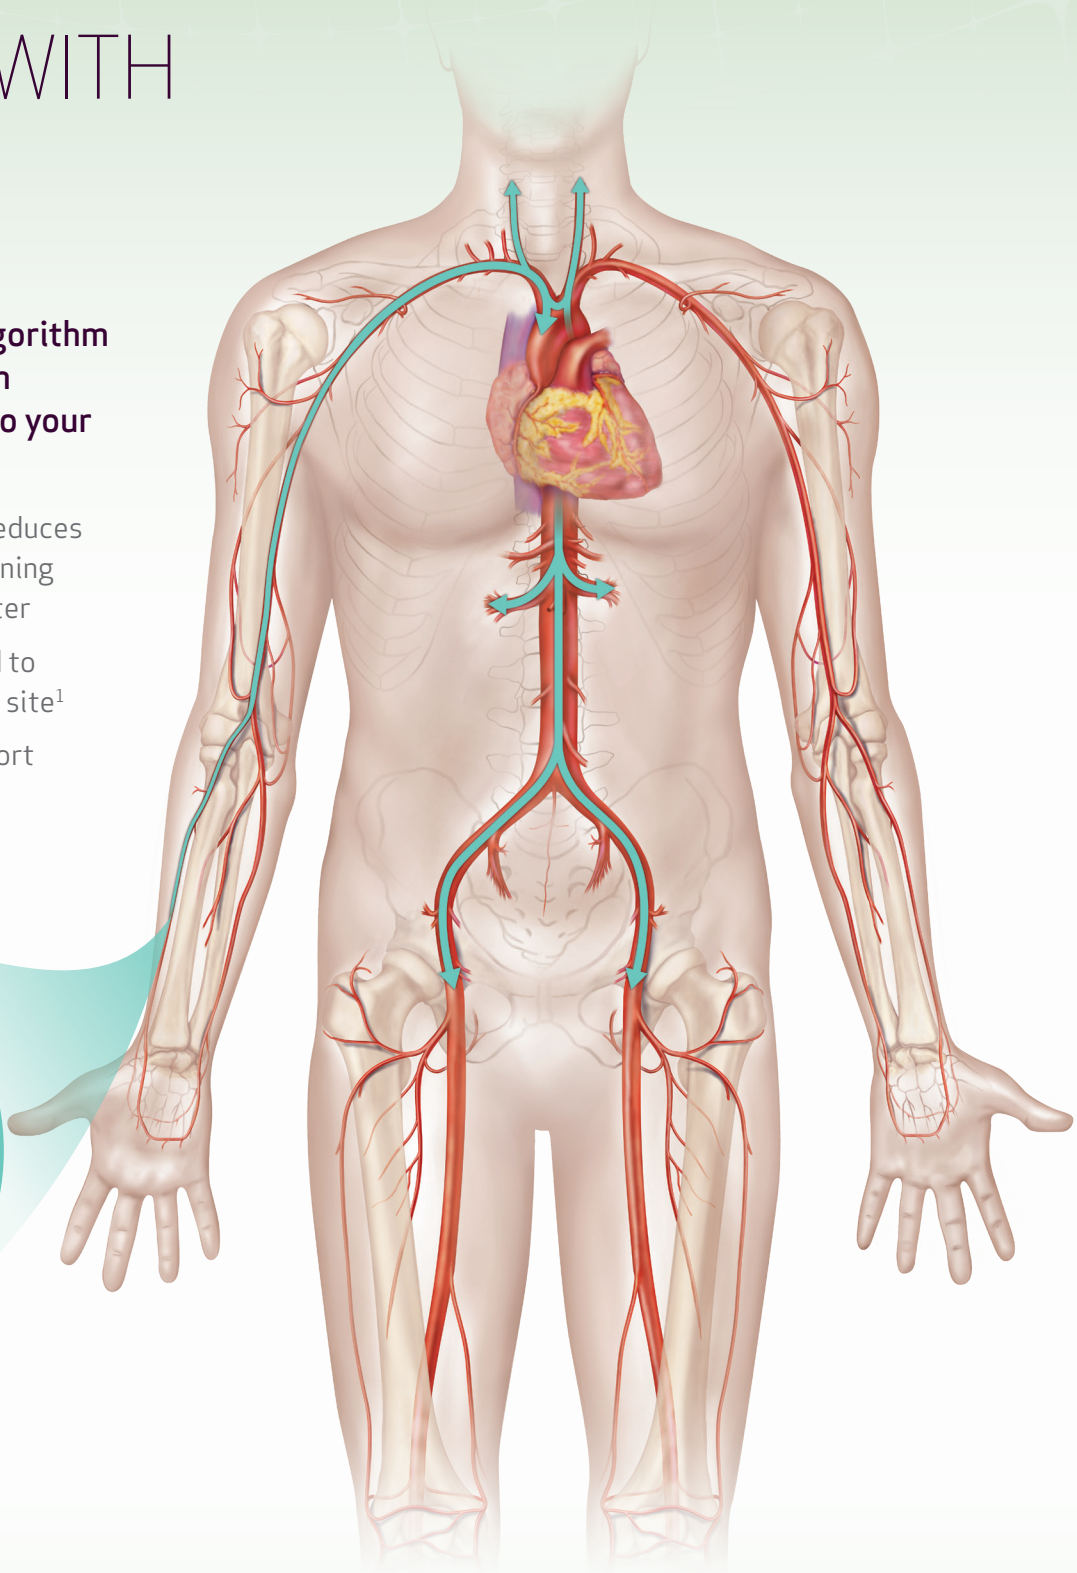

TERUMO. **YOUR** RADIAL **EDGE.**

TERUMO
INTERVENTIONAL SYSTEMS

[a] R2P™ DESTINATION SLENDER™ Guiding Sheath is not intended for discrete placement within the coronary or neuro vasculature.

PUSHING BOUNDARIES

Terumo Interventional Systems is **committed to your success** with innovative procedural solutions and ongoing support for your most challenging cases.

We are relentlessly seeking new ways to help you apply effective solutions and achieve **better outcomes for more patients.**

R2P® Destination Slender®
Guiding Sheath

PRODUCT CODE	WORKING LENGTH	TOTAL LENGTH	FR SIZE	TIP SHAPE	SHEATH ID	SHEATH OD	DEAD SPACE VOLUME	MAX GUIDEWIRE OD
GS-R6ST1C75W	75 cm	80 cm	6 Fr	Straight	2.2 mm / 0.087"	2.5 mm / 0.100"	4.0 mL	0.038" (0.97 mm) max
GS-R6ST1C85W	85 cm	90 cm	6 Fr	Straight	2.2 mm / 0.087"	2.5 mm / 0.100"	4.5 mL	0.038" (0.97 mm) max
GS-R6ST1C95W	95 cm	100 cm	6 Fr	Straight	2.2 mm / 0.087"	2.5 mm / 0.100"	5.0 mL	0.038" (0.97 mm) max
GS-R6ST1C10W	105 cm	110 cm	6 Fr	Straight	2.2 mm / 0.087"	2.5 mm / 0.100"	5.5 mL	0.038" (0.97 mm) max
GS-R6ST1C12W	119 cm	124 cm	6 Fr	Straight	2.2 mm / 0.087"	2.5 mm / 0.100"	6.0 mL	0.038" (0.97 mm) max
GS-R6ST1C15W	149 cm	154 cm	6 Fr	Straight	2.2 mm / 0.087"	2.5 mm / 0.100"	7.0 mL	0.038" (0.97 mm) max

FIND OUT MORE

US: 800.888.3786
CA: 833.883.7866

US: terumois.com
CA: terumocanada.ca

Reference:
1. Data on file.

RX ONLY. The advertisement is directed to physicians only, and not to consumers. Refer to product labels and packaging insert for complete warnings, precautions, potential complications, and instructions for use. Products may not have regulatory approval in all countries. Please contact your local sales representative if you have questions about the availability of products in your area.

©2025 Terumo Medical Corporation and Terumo Medical Canada Inc. All rights reserved. All brand names are trademarks or registered trademarks of Terumo. PM-08235v2

TERUMO
INTERVENTIONAL SYSTEMS